

A 65nm Resonant Electro-Quasistatic 5-240uW Human Whole-Body Powering and 2.19uW Communication SoC with Automatic Maximum Resonant Power Tracking

Nirmoy Modak, Debayan Das, Mayukh Nath, Baibhab Chatterjee,
Gaurav Kumar K, Shovan Maity, Shreyas Sen
Purdue University, United States

Applications like Connected Healthcare through physiological signal monitoring and Secure Authentication using wearable keys can benefit greatly from battery-less operation. Low power communication along with energy harvesting is critical to sustain such perpetual battery-less operation. Previous studies have used techniques such as Tribo-Electric, Piezo-Electric, RF energy harvesting for Body Area Network devices, but they are restricted to on-body node placements. Human body channel is known to be a promising alternative to wireless radio wave communication for low power operation [1-4], through Human Body Communication, as well as very recently as a medium for power transfer through body coupled power transfer [5]. However, channel length (L) dependency of the received power makes it inefficient for $L > 40\text{cm}$. There have also been a few studies for low power communication through the human body, but none of them could provide sustainable battery-less operation. In this paper, we utilize Resonant Electro Quasi-Static Human Body Communication (Res-EQS HBC) with Maximum Resonance Power Tracking (MRPT) to enable channel length independent whole-body communication and powering (Fig.1). We design the first system to simultaneously transfer Power and Data between a HUB device and a wearable through the human body to enable battery-less operation. Measurement results show 240uW, 28uW and 5uW power transfer through the body in a Machine-Machine (large devices with strong ground connection) Tabletop (small devices kept on a table, as in [5]) and Wearable-Wearable (small form factor battery operated devices) scenario respectively, independent of body channel length, while enabling communication with a power consumption of only 2.19uW. This enables $>25\times$ more power transfer with $>100\times$ more efficiency compared to [5] for Tabletop and 100cm Body distance by utilizing the benefits of EQS. The MRPT loop automatically tracks device and posture dependent resonance point changes to maximize power transfer in all cases.

In the EQS regime, signal wavelength is significantly larger than the human body-size, enabling channel length independent loss and physically secure communication through signal confinement. The parasitic capacitances associated with the forward (device cap C_p) and return path (C_{ret}) are the primary contributors to channel loss (Fig.2) [1]. Previous studies primarily used 50 Ω receiver termination, resulting in ~80dB loss in the MHz range. EQS HBC utilizes high impedance termination [4] to reduce the channel loss to the 40-60dB, which is sufficient for communication but not powering. Resonant cancellation of the parasitic capacitances (Fig. 2) further reduces the channel loss to ~20dB, enabling whole body power transfer, for the first time, due to constant channel loss across the body. Series Resonance (HUB side) cancels C_p and boosts the transmitted voltage by a factor Q , increasing V_{TX} , improving whole-body power delivery. Simultaneous Parallel Resonance at the receiver helps to cancel C_L , C_{ret} and improves V_{RX} , providing a Q^4 boost in maximum received power ($P_{RX,max}$), making it ideal choice for HUB to NODE powering. For Communication, however, the FoM V_{RX}/P_{TX} , is maximized with Parallel Resonance at both ends, allowing a Q^3 boost, due to exhibiting a high impedance and hence transmitter current minimum at resonance, which helps transmitter power to be reduced by 33%, compared to simple EQS TX with 30pF load (Fig.3).

The resonant frequency is highly dependent on Device cap (C_p), return path cap (C_{ret}) and body cap (C_{Body}), which exhibits significant inter-device, posture-dependent and inter-human variability. This necessitates an MRPT loop to ensure maximum power delivery at all cases (Fig. 2). The HUB uses a dedicated frequency scanning phase before transmit phase to lock the resonant frequency automatically before power transmission, ensuring high P_{RX} and efficiency(η).

Fig. 3 shows the overall system architecture for the HUB and NODE. The battery-operated HUB consists of a Power Transmitter (series resonance) and a TRx link (parallel resonance). An on chip digitally controlled current steering oscillator generates the duty cycled corrected clock (0.1-5MHz) during both the scanning and


transmission phase. A fully synthesizable digital controller (HUB TX Unit) coordinates scanning and transmit phase for powering, and communication. An automatic feedback loop (MRPT) samples the peak value of the transmitted signal during scanning phase through a capacitive divider network and a peak detector consisting of a passive Envelope Detector (ED) followed by a sampler. Sampling and peak comparison between successive frames is done using a 32-bit shift register and a 16-bit counter. The receiver side stores the incoming power on a capacitor (Fig. 5) enabling perpetual NODE

The SoC is fabricated in 65nm CMOS technology (Area = 0.13mm²). Fig.4 shows measured results on how series resonance at HUB Tx helps maximize transmit voltage and hence P_{TX} , P_{RX} and η are shown as function of HUB TX supply voltage for Machine-Machine and Tabletop cases. The maximum received power is measured by varying the resistive component of the load at the receiver end. The peak received power in Machine-Machine, Tabletop and Wearable-Wearable scenario is 240uW (RL=1k Ω) with 37% efficiency, 28uW (RL=20k Ω) with 3% efficiency and 5uW(80k Ω) with 7% efficiency, respectively. Machine-Machine is most efficient with Series-EQS (no C_{ret}), and Tabletop is most-efficient with Series-Par Resonance. The Comm Tx consumes only 2.19uW power during data communication at parallel resonance while driving a 30pF load at 20Kbps DR and ~1MHz f_c , 33% lower than EQS-HBC due to cancellation of C_p . The HUB control unit and the digitally controlled starved oscillator consumes 0.3uW average power. The receiver operates at 10⁻⁵ BER at 20kbps data rate with a 0.55UI timing margin (Fig.5). The receiver shows a sensitivity of -60dBm (318uV) and -52dBm(794uV) with 1kbps and 20kbps data rate, respectively. At the lowest power mode, the receiver consumes only 72nW power. Powering and Data Communication timing waveforms (Fig.5) show automatic MRPT & successful demodulated data, respectively.

Fig.6 shows comparison with other works (either only powering or only communication). This design achieves $\eta=37\%$ for machine-machine, $\eta=3\%$ for a tabletop and $\eta=7\%$ for a wearable-wearable interaction scenario, independent of channel length (i.e. whole-body powering) and $>4.5\times$ lower maximum transmitted power, increasing safety. This is $>100\times$ improvement in body coupled power transfer efficiency and $>10\times$ improvement in peak power transfer for longer channel lengths as shown in the comparison table in Fig.6. The current design utilizes the body channel for the first time to enable simultaneous data communication, at 2.19 μ W power budget, along with whole-body power transfer making battery-less perpetual body nodes a reality.

References:

- [1] S. Maity et al., "Bio-Physical Modeling, Characterization, and Optimization of Electro-Quasistatic Human Body Communication," TBME 2019.
- [2] J. Lee et al., "A 60Mb/s Wideband BCC Transceiver with 150pJ/b Rx and 31pJ/b Tx for Emerging Wearable Applications" ISSCC 2015.
- [3] J. Park et al., "17.6 a sub-40W 5mb/s magnetic human body communication transceiver demonstrating trans-body delivery of high-fidelity audio to a wearable in-ear headphone" ISSCC 2019.
- [4] S. Maity et al. "A 415nW Physically and Mathematically Secure Electro-Quasistatic HBC Node in 65nm CMOS for Authentication and Medical Applications" CICC 2020.
- [5] J. Li et al., "Human-Body-Coupled Power-Delivery and Ambient-Energy-Harvesting ICs for a Full-Body-Area Power Sustainability" ISSCC 2020.



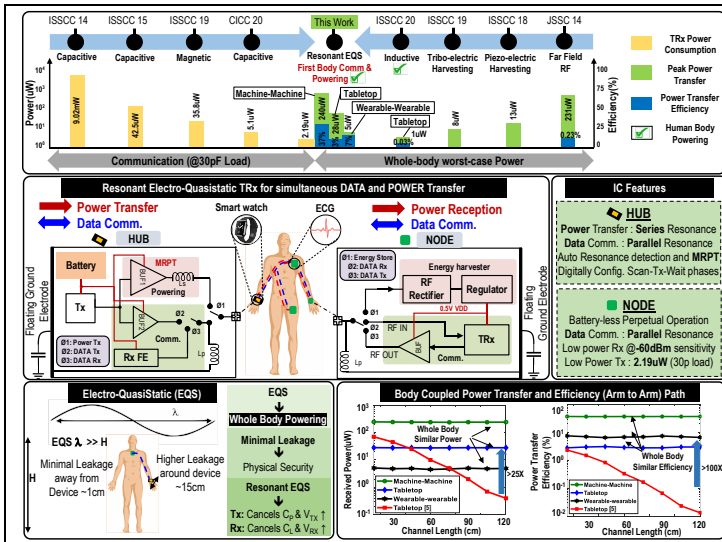


Fig. 1. Resonant Electro Quasi-Static Human Whole-Body Powering and Communication: Detailed architecture and comparison with previous Body Area Network communication and powering.

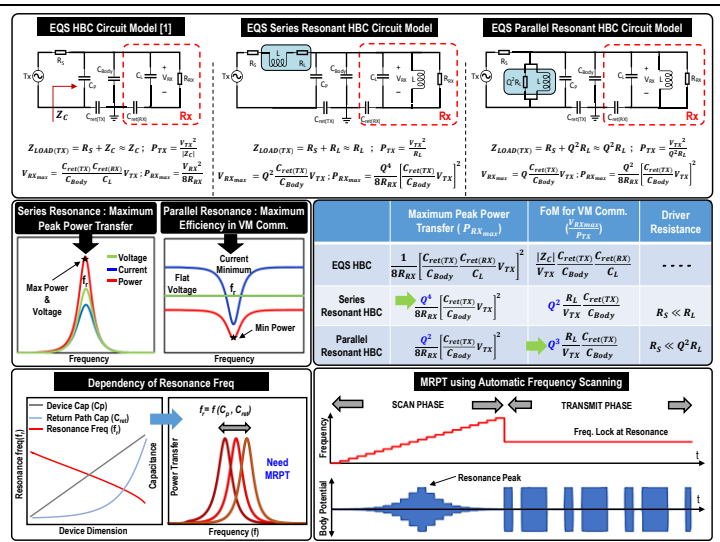


Fig. 2. Theoretical analysis of voltage & power transfer of different resonant techniques. Variation of resonant frequency with physical parameters and auto Maximum Resonant Power Tracking (MRPT).

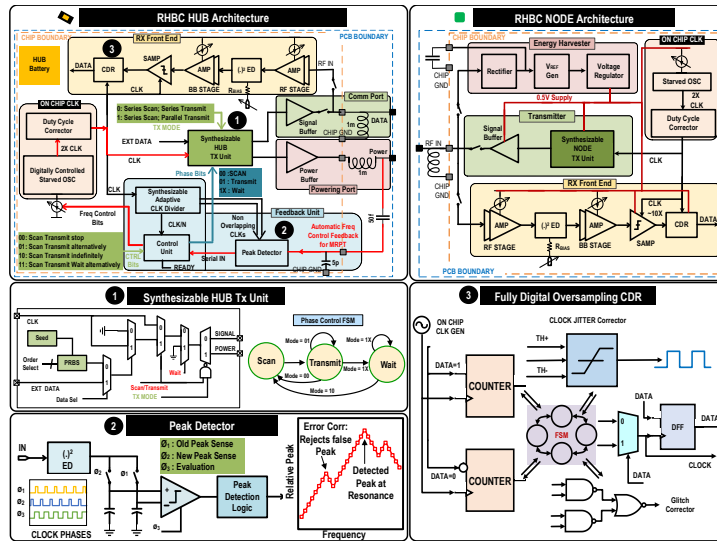


Fig. 3. Overall architecture of the Hub and the Node device. Detailed design of the Hub Tx unit, peak detector, and the oversampling Clock Data Recovery circuit.

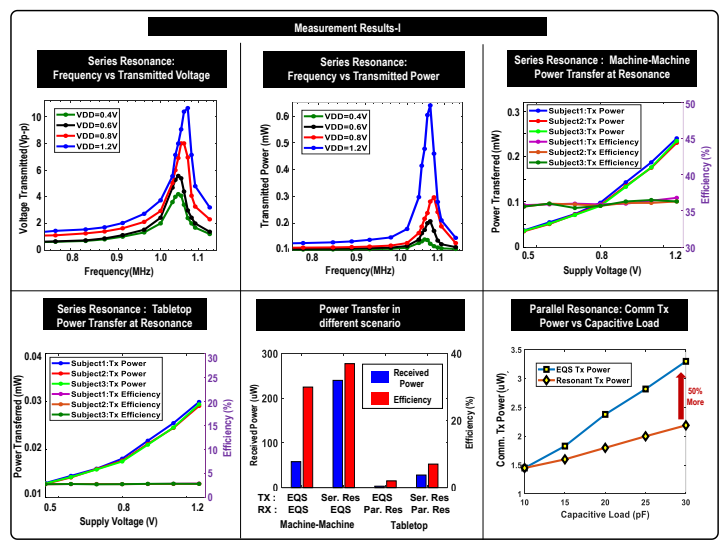


Fig. 4. Measured received power & efficiency of power transmission. Lesser transmitter power consumption during communication at parallel resonance due to cancellation of the load capacitance.

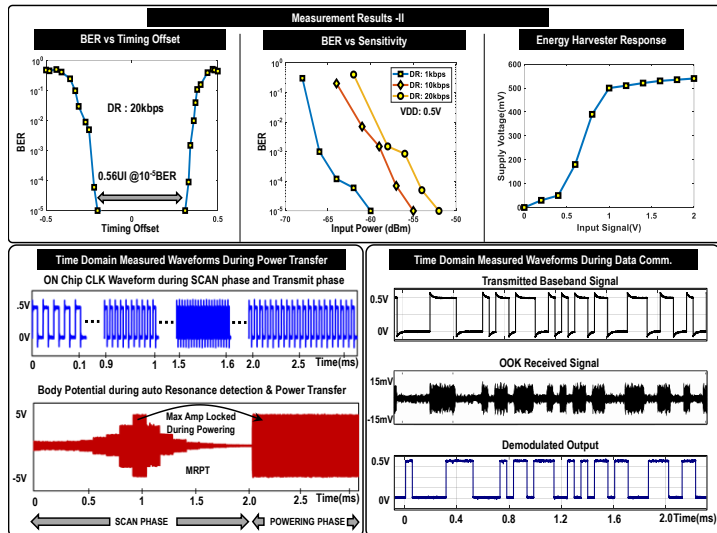


Fig. 5. Receiver bathtub curve & sensitivity analysis of the receiver. Time domain snapshot of the scanning phase at the transmitter and data communication between transmitter and receiver.

Comparison Table with State-of-the-Art HBC Transceivers and Energy Harvesting Techniques for Wearables									
Powering & Comm	This Work	Only Powering				Only Communication			
		J. Li ISSCC '20	M. Meng ISSCC '18	L. Xia JSSC '14	S. Maity CICC '19	H. Cho ISSCC '15	J. Park ISSCC '19	J. Lee ISSCC '14	
Technique	Resonant EQS (Body Coupled)	Body-coupled + Ambient	Tribo-electric Harvesting	Piezoelectric Harvesting	Capacitive	Capacitive	Magnetic	Capacitive	
Process	65nm CMOS	40nm CMOS	180nm BCD	0.35μm CMOS	65nm CMOS	65nm CMOS	65nm CMOS	65nm CMOS	
Operating Freq	0.5-2 MHz	40 MHz Tx 50/60 Hz	100 Hz	90-160 Hz	904.5 MHz	0.1-1 MHz	10/13.56 MHz	40 MHz	40-80 MHz
Human Body Powering	Yes	Yes	No	No	No				
Power Delivered	240 uW (Machine-Machine) 28 uW (Tabletop), Whole Body 5 uW (Wearable-Wearable)	1 uW (100cm, Tabletop) 100 uW (~cm)	2-8 uW	2-13 uW	231.6 uW (~3m)				
Transmit Power	650 uW (Max) → Safer	3mW	NA	NA	20 dBm				
Efficiency	37% (Machine-Machine) 3% (Tabletop) 7% (Wearable-Wearable)	0.03-3.33%	NA	NA	0.232%				
Coverage	Full body (Distance Independent)	Joint and feet	Limbs		0.9-9m (antenna dependent)				
Modulation	OOK				OOK	OOK	OOK	Walsh Coding	
Supply Voltage	0.5				0.5	0.8	0.6	1.1	
Data Rate	1-20Kbps				1-20Kbps	100Kbps	5 Mbps	60 Mbps	
Tx Power	1.3uW (10p load) 1.5uW (20p load) 2.19uW (30p load)				3.7 uW @ 1MHz f _c (30p load)	21 uW	35.8uW	1.85mW	
Rx Power	72mW (with on-chip OSC and CDR)				1.4 uW	42.5 uW	24uW	9.02mW	
Sensitivity	-60 dBm @ 10 ⁻⁵ BER				-64dBm @ 10 ⁻⁵ BER	-60 dBm @ 10 ⁻⁵ BER	-56 dBm @ 10 ⁻⁵ BER	-58 dBm @ <10 ⁻⁵ BER	

Fig. 6. Comparison with state-of-the-art HBC Transceivers and energy harvesting techniques, showing the first work to simultaneously transmit power and communicate data.